This Page Is Inserted by IFW Operations and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.



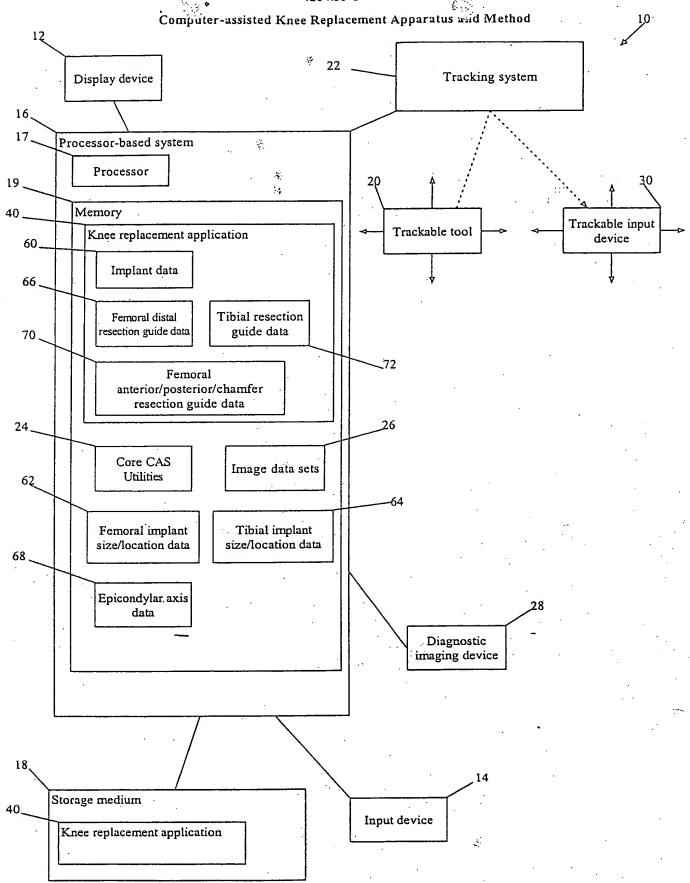


Figure 1

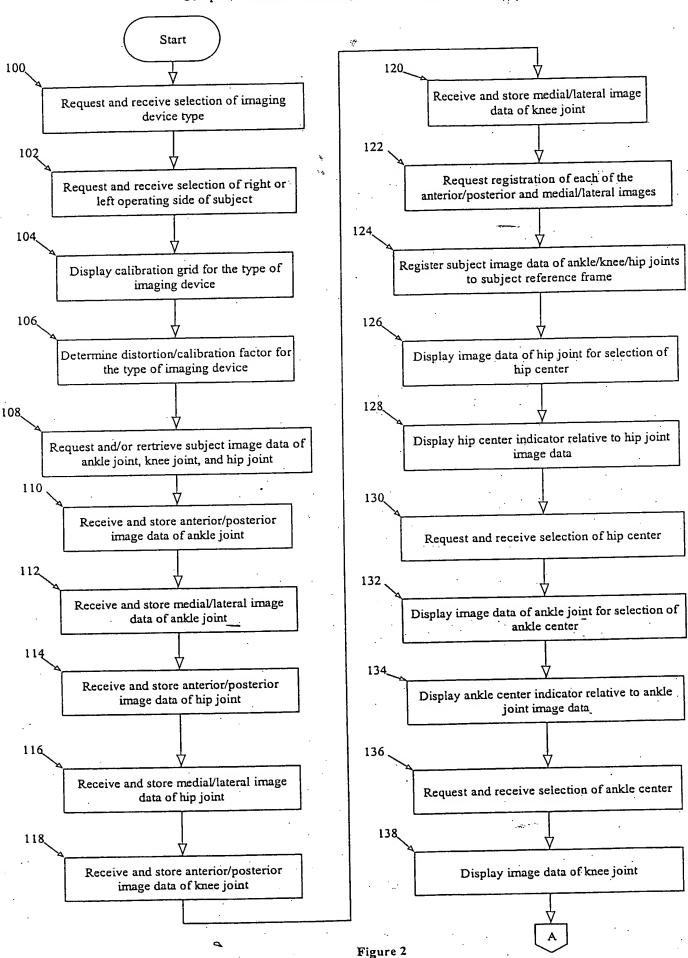

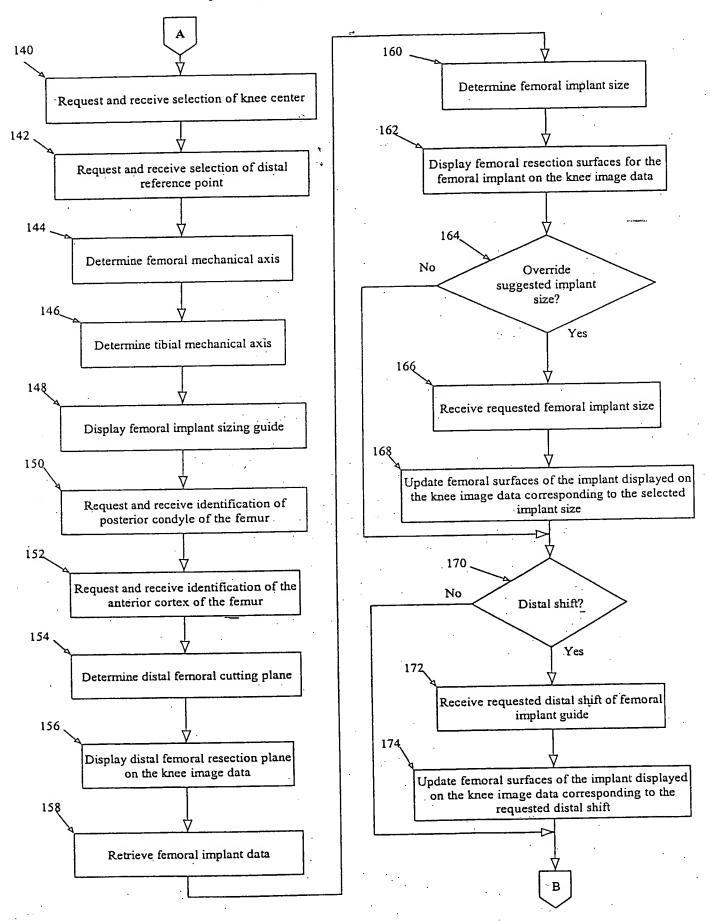

.Figure 2 (continued)

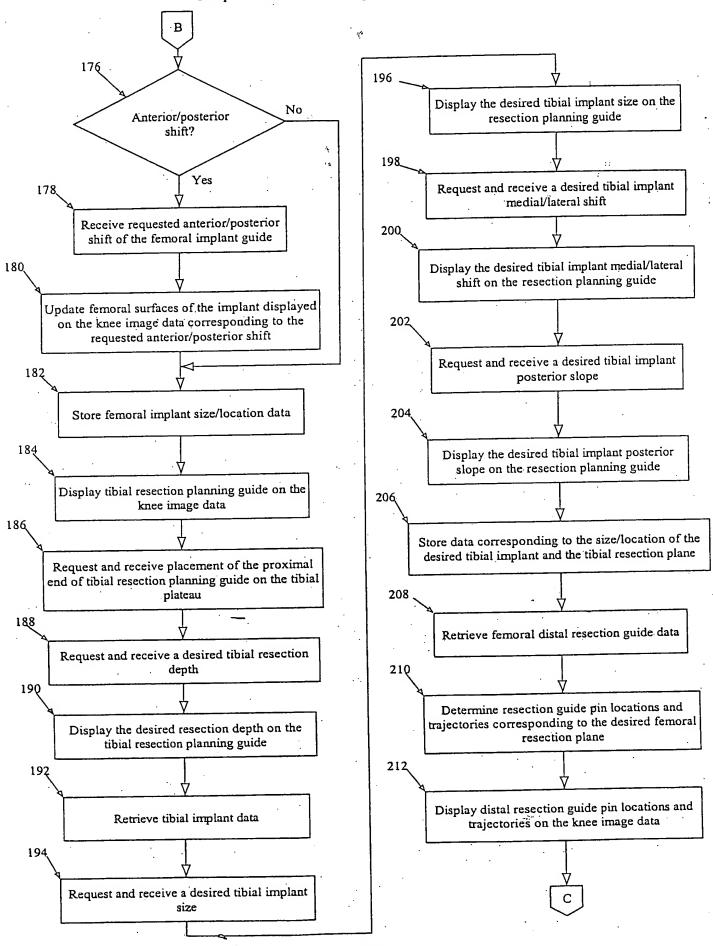


Figure 2 (continued)

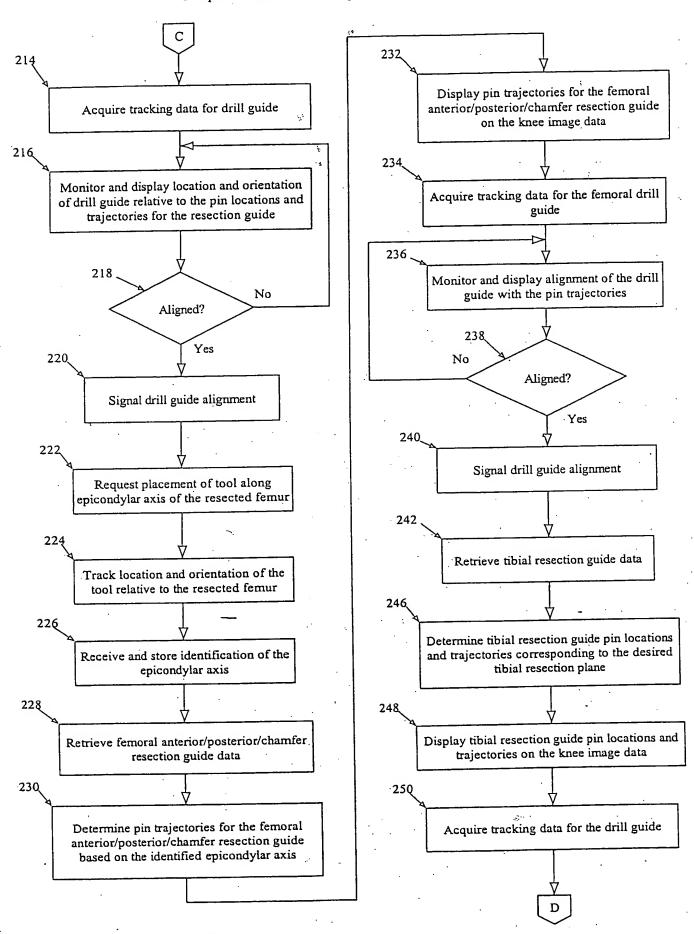


Figure 2 (continued)



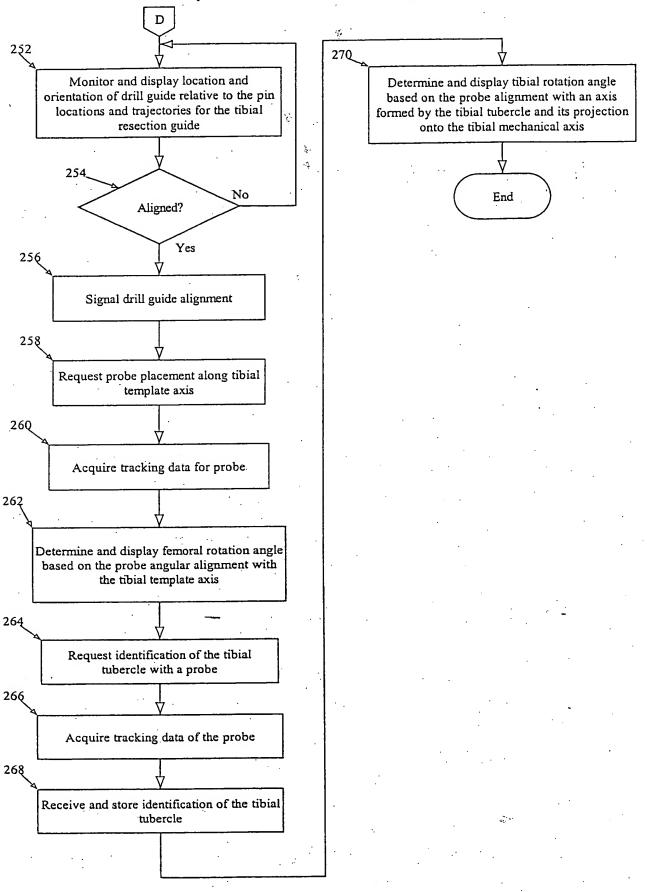


Figure 2 (continued)

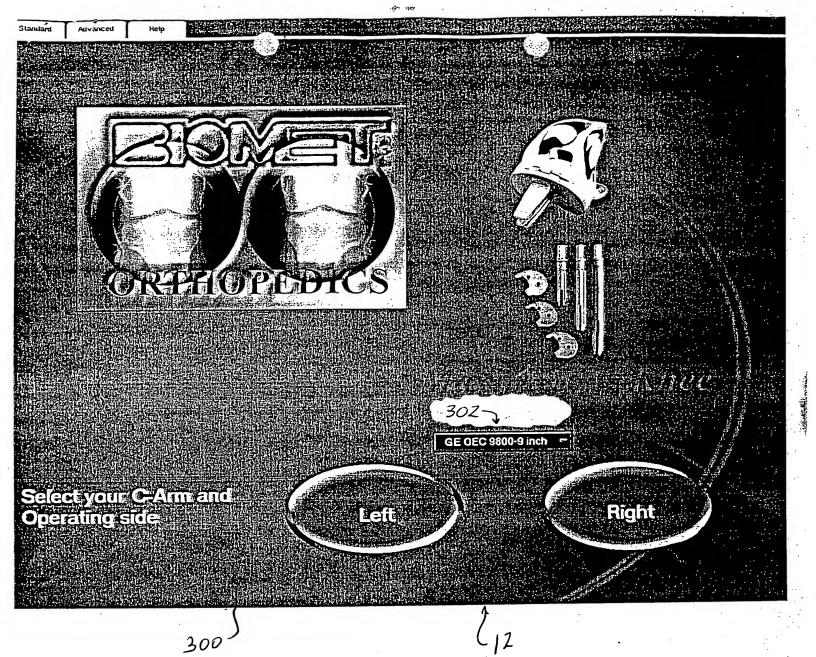

4204.33-1

FIG. 3

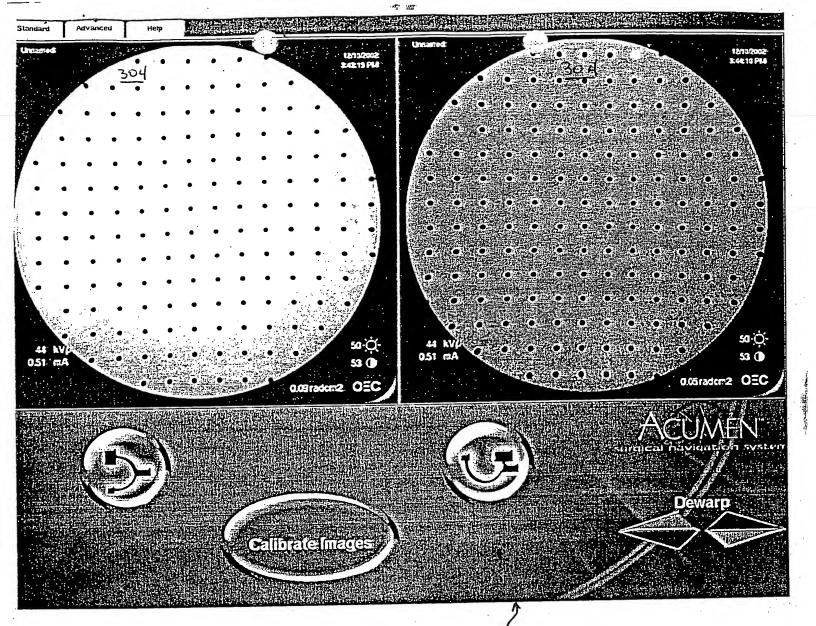

4204.33-1

FIG. 4

4204.33-1

. . .

4204.33-1

Place Ankle Center

//-

Ankle Center

12

4204.33-l

Computer-assisted Knee Replacement Apparatus and Method

FIG. 7

4204.33-1

4204.33-1

4204.33-1

4204.33-1

4204.33-1

4204.33-1

4204.33-1

4204.33-1

4204.33-1

Computer-Assisted Knee Replacement Apparatus and Method

Figure 16

12

4204.33-1

Computer-Assisted Knee Replacement Apparatus and Method

Figure 17